



AENSI Journals

Advances in Environmental Biology

Journal home page: <http://www.aensiweb.com/aeb.html>



## The Corrosion Studies of Powder Metallurgy Co-Cr-Mo (F-75) Alloy

<sup>1</sup>Zuraidawani Che Daud, <sup>2</sup>Shamsul Baharin Jamaludin, <sup>3</sup>Mohd Nazree Derman, <sup>4</sup>Juyana A. Wahab

<sup>1,2</sup>Sustainable Engineering Research Cluster, Universiti Malaysia Perlis, Blok B, Taman Pertiwi Indah, Seriab, 01000 Kangar, Perlis, Malaysia

<sup>3</sup>Institute of Nano Electronic Engineering, Lot 106, 108 & 110, Blok A, Taman Pertiwi Indah, Jalan Kangar-Alor Setar, Seriab 01000 Kangar, Perlis, Malaysia.

<sup>4</sup>School of Materials Engineering, Universiti Malaysia Perlis, Kompleks Pusat Pengajian Jejawi 2, 02600 Jejawi, Arau, Perlis.

### ARTICLE INFO

#### Article history:

Received 11 September 2013

Received in revised form 21

November 2013

Accepted 25 November 2013

Available online 3 December 2013

#### Key words:

Co-Cr-Mo (F-75) Alloy, Immersion test, Powder Metallurgy

### ABSTRACT

Co-Cr-Mo (F-75) alloy was investigated for biomedical application due to its mechanical properties and good corrosion resistance. This study has been focusing on the corrosion behavior of PM Co-Cr-Mo alloy. The Co-Cr-Mo powder were first blended with binder using rotation mill and compacted using uniaxial cold press to a pellet shape and then sintered at two sintering temperatures (1300°C and 1350°C) with 90 minutes of sintering time. Immersion test was carried out in a water bath with maintaining the temperature at 37°C for 90 days. The results show that sample sintered at 1350°C has the lowest mpy result after 90 days immersed in 0.9% sodium chloride.

© 2013 AENSI Publisher All rights reserved.

**To Cite This Article:** Zuraidawani Che Daud, Shamsul Baharin Jamaludin, Mohd Nazree Derman, Juyana A. Wahab., The Corrosion Studies of Powder Metallurgy Co-Cr-Mo (F-75) Alloy. *Adv. Environ. Biol.*, 7(12), 3716-3719, 2013.

## INTRODUCTION

Implants are fabricated from a wide variety of materials, including metals, polymers, ceramics and their composites. Among these materials, metals are an important group. Stainless steel, Co-Cr alloys and Ti alloys are the common metals used in orthopaedics applications. Alloys selection for a specific application has depended upon a variety of design criteria, including biocompatibility, corrosion resistance, tensile strength, fatigue strength, modulus wear resistance, processing and also cost [1-2]. In metallic biomaterials, corrosion is the unwanted chemical reaction of a metal with its environment. Tissue fluid in the human body contains water, dissolved oxygen, proteins, and various ions such as chloride and hydroxide. As a result, the human body presents a very aggressive environment for metals used for implantation. Therefore, corrosion resistance of a metallic implant material is consequently an important aspect of its biocompatibility.

Cobalt based alloys are highly resistant to corrosion even in chloride environment due to spontaneous formation of thin passive oxide layer within human body environment [3-4]. Until recently, its unique properties have attracted attention. Many previous studies tested *in vitro* corrosion characteristics. Hodgson et al. [5] investigated the behaviour of a Co-Cr-Mo alloy under simulated body conditions. They focused on the electrochemical properties of the alloy and the relevant mechanism in the passive and transpassive states. They have reported that the passive film on Co-Cr-Mo changed in composition and thickness with both potential and time. They also stated that the passive behaviour of the Co-Cr-Mo alloy is due to a formation an oxide film highly enriched with Cr ( $\approx 90\%$  Cr oxides) on the alloy surface. Krasicka-Cydzik et al. [6] have done corrosion testing on the sintered samples made of Co-Cr-Mo alloy for surgical applications. They have found that the repressing and subsequent heat treatment applied to the sintered samples made of the Co-Cr-Mo alloy powder influenced significantly and beneficially their microstructure, porosity and corrosion resistance. Thus, the aim of this work is to study the corrosion behavior of sintered PM Co-Cr-Mo (F-75) alloy.

### Methodology:

Co-Cr-Mo powder with average size 8.8  $\mu\text{m}$  was used as starting materials. This powder was supplied by Sandvik Osprey Ltd, UK. The samples were fabricated using a powder metallurgy route in which Co-Cr-Mo

**Corresponding Author:** Zuraidawani Che Daud, Sustainable Engineering Research Cluster, Universiti Malaysia Perlis, Blok B, Taman Pertiwi Indah, Seriab, 01000 Kangar, Perlis, Malaysia  
E-mail: zuraidawani@unimap.edu.my,

powders and 2 wt. % of stearic acid (as a binder) were blended for 30 min. The mixed powders were poured into a die with 13 mm diameter and compacted using uniaxially cold press at a pressure of 500 MPa. The green compacts were sintered using WEBB 84 furnace at two different temperatures; 1300 °C and 1350 °C and known as sample A<sub>1</sub> and sample A<sub>2</sub> respectively. The samples were sintered for 90 minutes in argon atmosphere. The bulk density and apparent porosities of each of the samples were determined using the Archimedes principle. The sintered samples were polished according to the standard preparation of metallographic specimen. Samples were then immersed in 0.9 % NaCl solution at 37°C for 90 days. The corrosion rate by mils per year expression was calculated according to the ASTM G31, Eq. [1],

$$mpy = \frac{KW}{DAT} \quad (1)$$

where  $K$  is the constant,  $W$  is mass loss (g),  $D$  is density (g/cm<sup>3</sup>),  $A$  is area of sample (cm<sup>2</sup>) and  $T$  is time of exposure (hr).

The microstructures of the sample before and after immersion test were observed under optical microscope (Olympus BX41M).

## RESULT AND DISCUSSION

Table 1 shows the properties of PM Co-Cr-Mo alloy sintered at 1300°C and 1350°C respectively with 90 minutes of sintering time. It is seen that the bulk density increased with increasing the sintering temperatures. Meanwhile an opposite trend was obtained in properties of apparent porosity.

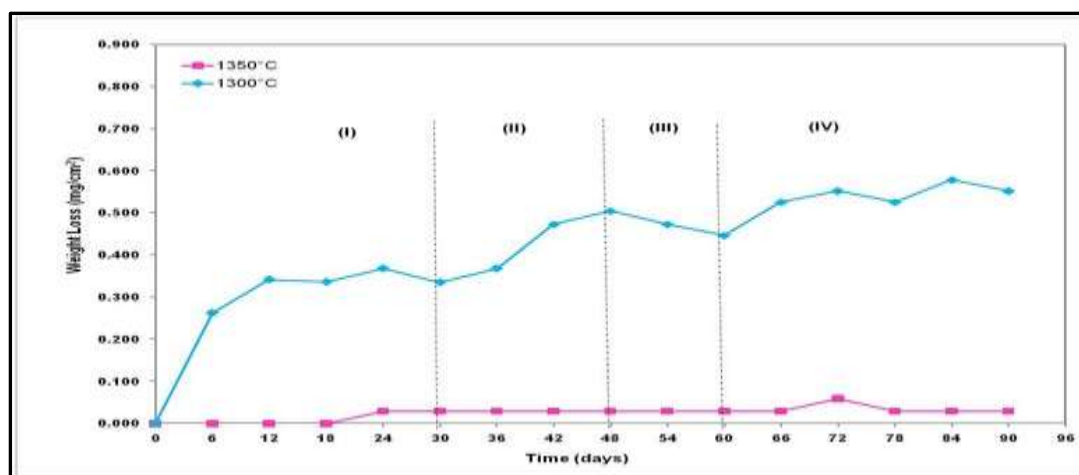
Fig. 1 shows the trend of weight loss per area as a function of time for 2 samples with different sintering temperatures (1300°C and 1350°C). It can be seen that, sample A<sub>1</sub> give the highest weight loss per area, meanwhile sample A<sub>2</sub> shows the lowest weight loss per area. To clarify the trend of each sample, the graph is divided into four parts.

Part (I) represents the value of weight loss per area in the range of 0 to 36 days of immersion. The graph plotted shows the weight loss per area were gradually increased started from 6 to 30 days. Part (II) illustrates the weight loss per area in the range of 30 to 48 days. Based on this part, the weight loss per area was drastically increased for samples A<sub>1</sub>. Part (III) in the range of 48 to 60 days of immersion; showing a drastically decrease in weight loss per area for samples A<sub>1</sub>. Meanwhile, the weight loss per area for sample A<sub>2</sub> remains consistent started from 24 up to 66 days of immersion. Part (IV) shows the weight loss per area in the range of 60 days to 90 days. Overall, the weight loss is found to be constant for all samples.

The results in Table 2 showed that the sample A<sub>1</sub> has the highest value (0.122 mpy) of corrosion rate and sample A<sub>2</sub> has the lowest value (0.006 mpy) of corrosion rate. Thus, sample A<sub>2</sub> has the highest corrosion resistance after completed 90 days of immersion test. In this study, the porosity was influenced the corrosion behavior of PM Co-Cr-Mo alloy.

**Table 1:** The properties of PM Co-Cr-Mo alloy sintered at different sintering temperatures

Properties	Sintering temperatures	
	1300°C	1350°C
Bulk density (g/cm <sup>3</sup> )	7.23	7.49
Apparent porosity (%)	1.90	0.02

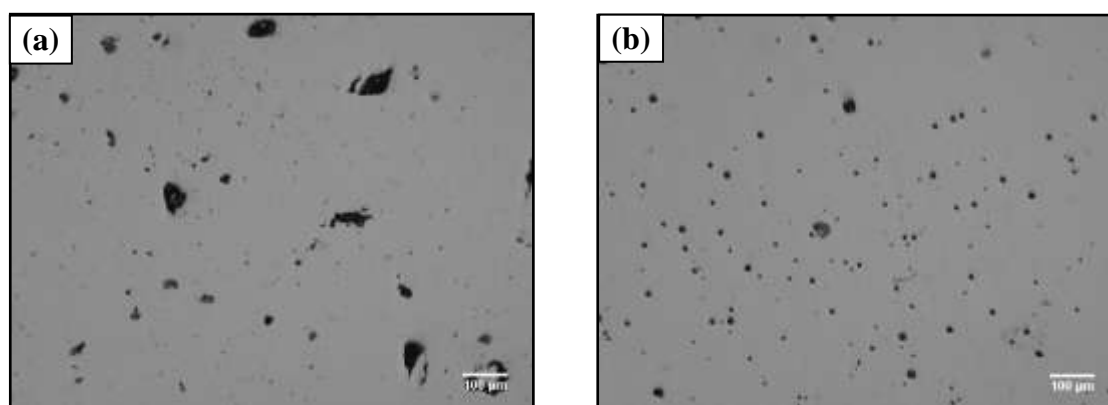
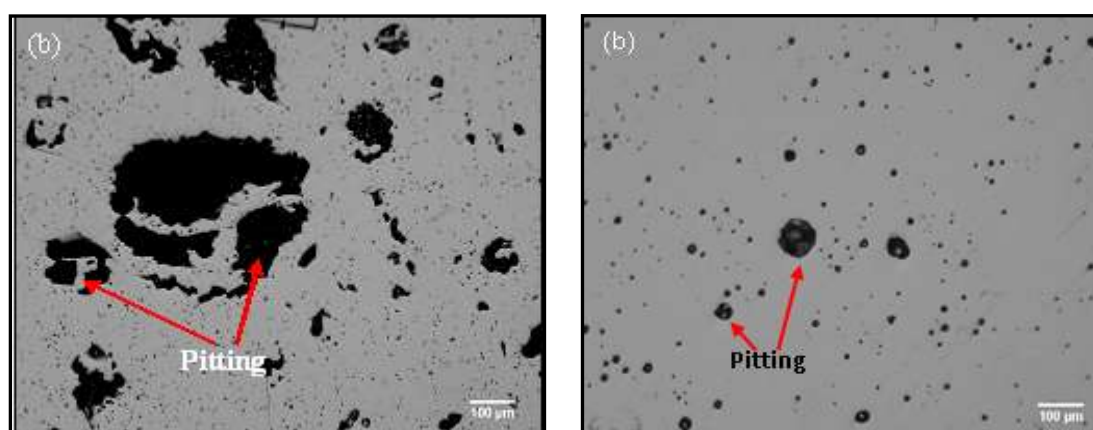


**Fig. 1:** The weight loss in mg/cm<sup>2</sup> for samples A<sub>1</sub> and A<sub>2</sub> after 90 days

**Table 2:** The value of corrosion rate (mpy) after completed 90 days duration of immersion test.

Samples with different temperatures	Corrosion rate (mpy)
Sample A <sub>1</sub>	0.122
Sample A <sub>2</sub>	0.006

From the observation, it was shown that the holes or pores are observed at all sintered samples before immersed in 0.9% NaCl solution (Fig. 2). After completed 90 days of immersion test, the pores become bigger compared to the samples before immersion. Fig. 3 exhibits optical micrographs of the samples after completed 90 days of immersion test. It can be seen that the corrosion attacked in the pores area due to reaction of aggressive ions between samples and solution. Because of that, the smaller pores become bigger with an irregular shape and spherical shapes were observed in the samples after completed immersion test. Virtanen et al. [7] stated that the corrosion behaviour is influenced by a wide variety of factors, including the material itself (the chemical composition, microstructure, surface condition) and the surroundings (temperature, O<sub>2</sub> content). Changes in these variables can influence the mode and rate of metal ion release. The corrosion attacks in all samples can be categorised under pitting corrosion. Generally, it occurs when discrete areas of material undergo rapid attack while most of the adjacent surface remains virtually unaffected. It is generally associated with specific ion in solution, which the most common is chloride [8-9].

**Fig. 2:** Optical micrograph of 2 different samples before an immersion test (a) Sample A<sub>1</sub>, and (b) Sample A<sub>2</sub>**Fig. 3:** Optical micrograph of 2 different samples after an immersion test (a) Sample A<sub>1</sub>, and (b) Sample A<sub>2</sub>**Conclusion:**

Corrosion behavior indicated that the sample sintered at temperature 1350 °C (sample A<sub>2</sub>) has the lowest mpy value after 90 days immersed in 0.9% sodium chloride solution. Thus, this sample has good corrosion resistance compared to sample sintered at 1300°C (sample A<sub>1</sub>).

**ACKNOWLEDGEMENTS**

This work is supported by Science Fund Grant (No 9005-00008).

**REFERENCES**

- [1] Walter, M., 2006. Benefits of P/M Processed Cobalt-Based Alloy for Orthopaedic Medical Implants. Carpenter Technology Corp., Wyomissing, PA, USA.
- [2] Zuraidawani, C.D., and J.B. Shamsul, 2013. The Effect of Sintering on the Properties of Powder Metallurgy (PM) F-75 Alloy. *Advanced Material Research*, 795: 573-577.
- [3] Jacobs, J.J., J.L. Gilbert and R. M. Urban, 1998. Current Concept Review-Corrosion of Metal Orthopaedic Implants. *Journal of Bone & Joint Surgery*, 80: 268-282.
- [4] Nasab, M.B., and M.R Hassan, 2010. Metallic Biomaterials of Knee and Hip: A Review. *Trends Biomaterial Artificial Organ*, 24(1): 69-82.
- [5] Hodgson, A.W.E., S. Kurz, S. Virtanen, V. Fervel, C.O.A. Olsson and S. Mischler, 2004. Passive and Transpassive Behaviour of CoCrMo in Simulated Biological Solutions. *Electrochimica Acta*, 49(13): 2167-2178.
- [6] Krasicka-Cydzik, E., Z. Oksiuta and J. R. Dabrowski, 2005. Corrosion Testing of Sintered Samples Made of the Co-Cr-Mo Alloy for Surgical Applications. *Journal of Materials Science: Materials in Medicine*, 16(3): 197-202.
- [7] Virtanen, S., I. Milosev, E. Gomez-Barrena, R. Trebse, J. Salo and Y.T. Konttinen, 2008. Special Modes of Corrosion under Physiological and Simulated Physiological Condition. *Acta Biomaterialia*, 4(3): 468-476.
- [8] Kamachimudali, U., T. Sridhar and B. Raj, 2003. Corrosion of Bio Implants. *Sadhana*, 28(3): 601-637.
- [9] Burstein, G.T., C. Liu and R.M. Souto, 2005. The Effect of Temperature on the Nucleation of Corrosion Pits on Titanium in Ringer's Physiological Solution. *Biomaterials*, 26: 245-256.